


Supplemental Digital Content 5: Supplemental Figure 2. The calibration curve of the model.

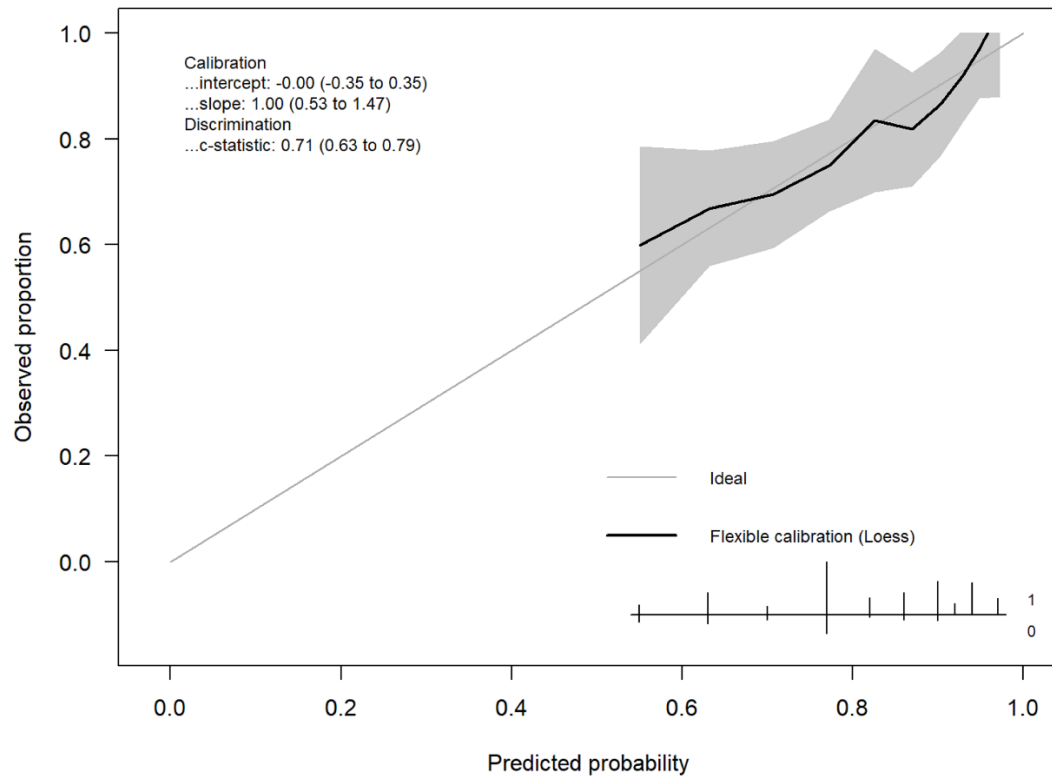

The calibration intercept was 0 (95% CI: -0.35 to 0.35) and the calibration slope was 1.00 (95%CI: 0.53 to 1.47) showing that on average, the model does not over- or underestimate risk.